


NOTE:

.118 WIDE SLOTS MUST BE ORIENTED 90° FROM ONE MOUNTING HOLE;

TOP VIEW:



600°C AIR OPERATION.

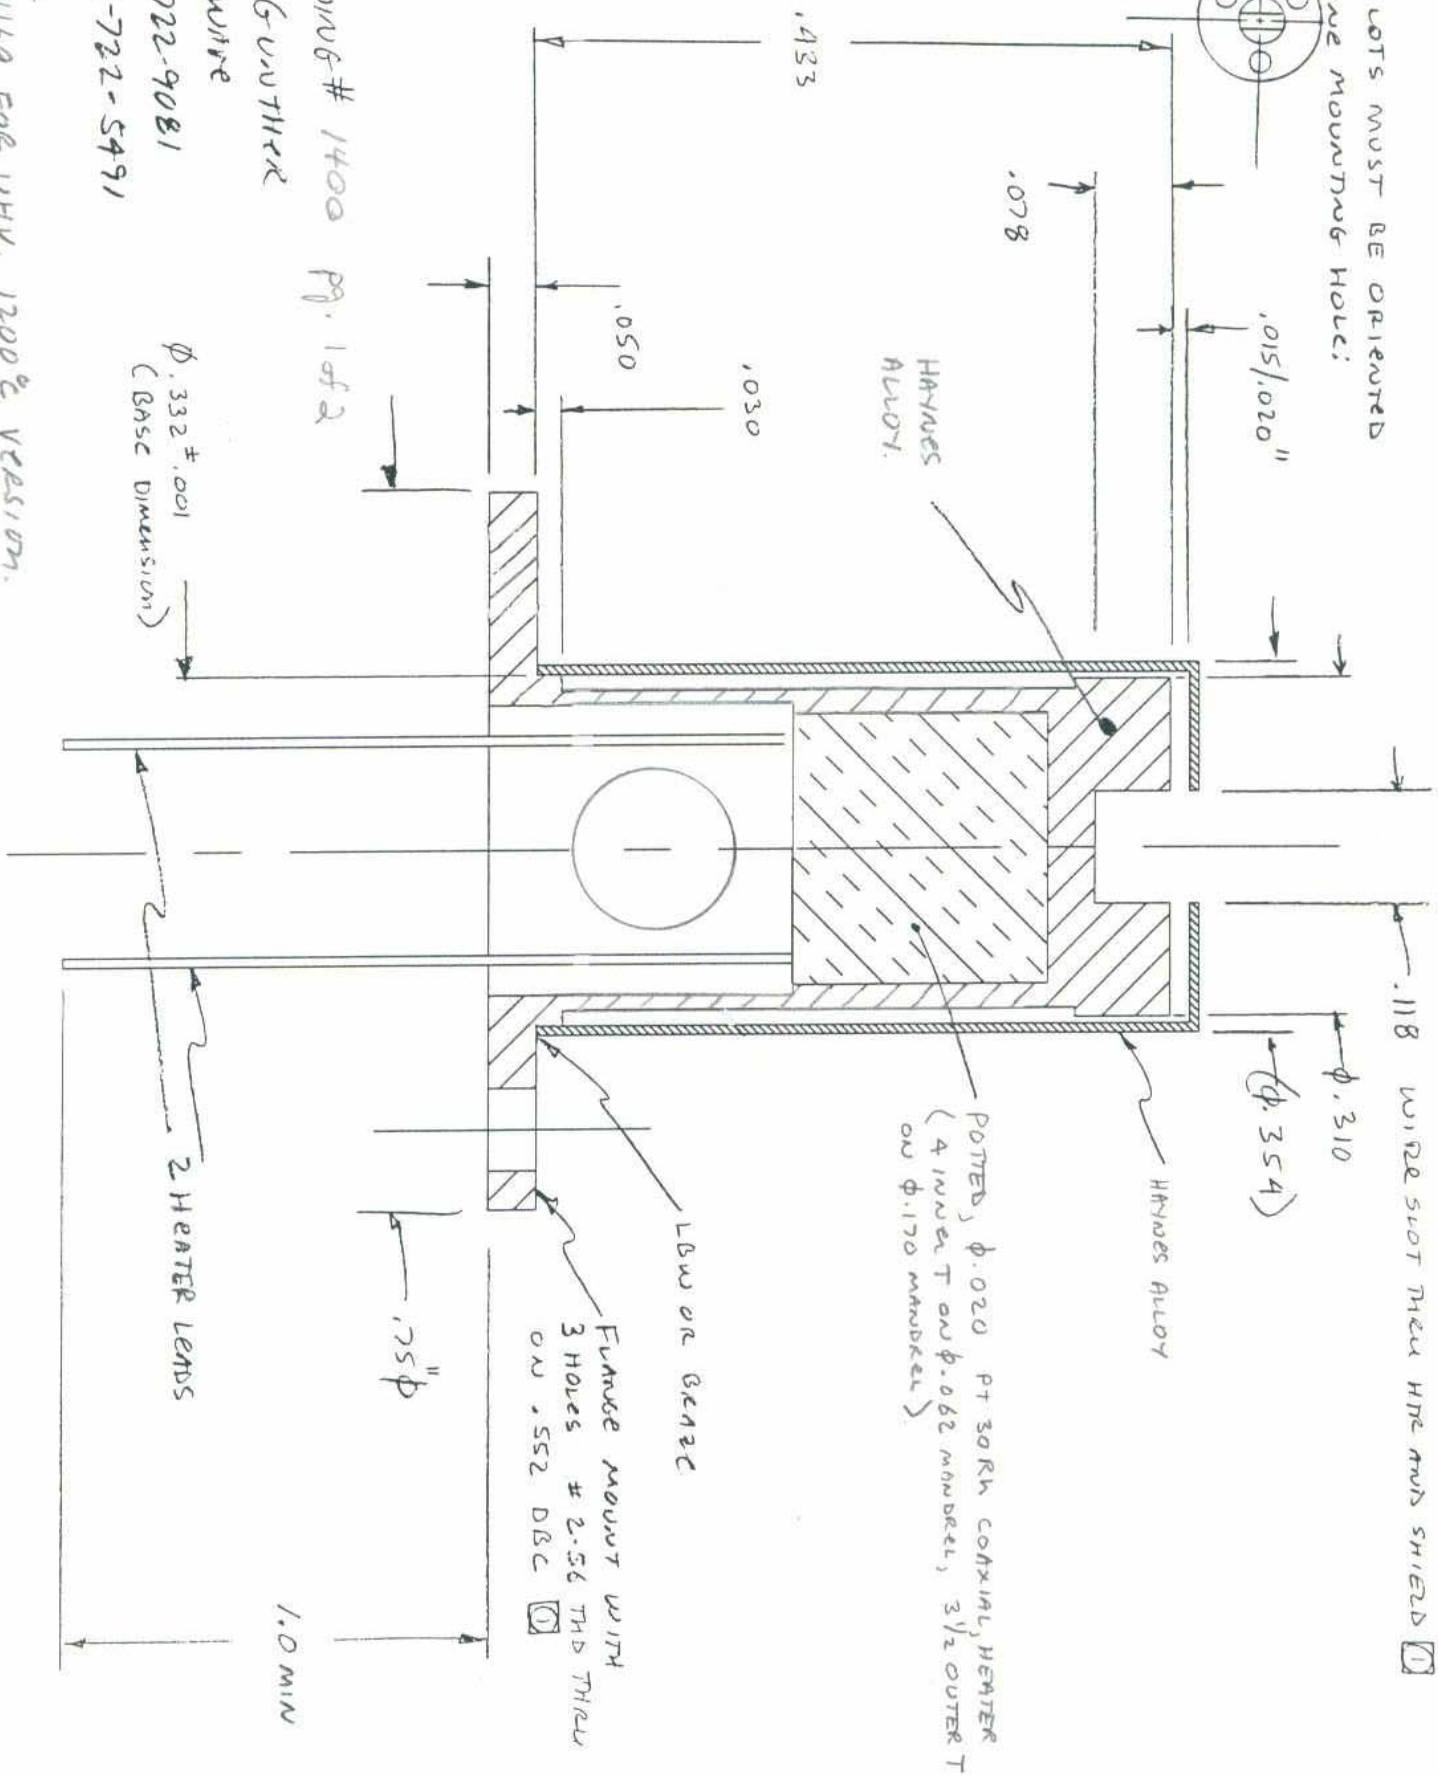

.118 WIRE SLOT THEN HTR AND SHIELD

φ .310

(φ .354)

POTTED, .020 PT BORN COAXIAL HEATER (4 INVERT AND .062 MINDEEL, 3 1/2 OUTER T ON .170 MINDEEL)

HAYNES ALLOY

LBU AIR BEARING

FLANGE MOUNT WITH 3 HOLES # 2.56 THD THRU ON .552 DISC

.75" φ

1.0 MIN

2 HEATER LEADS

φ .332 ± .001 (BASE DIMENSION)

DRAWING # 1400 Pg. 1 of 2
KIM GUNTHER
HEATHWARE
831-722-9081
FX 831-722-5491

SEE 10/169 FOR UHV, 1200°C VERSION.